Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 1 of 35



FIG.I

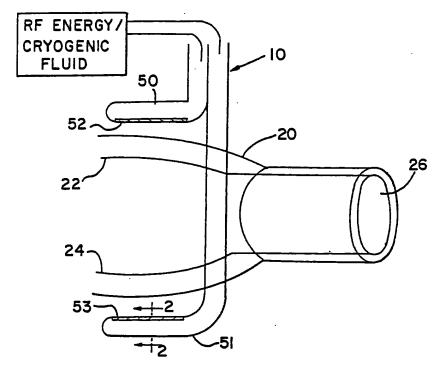


FIG.2




FIG. 3



FIG.4




FIG.5





FIG.6





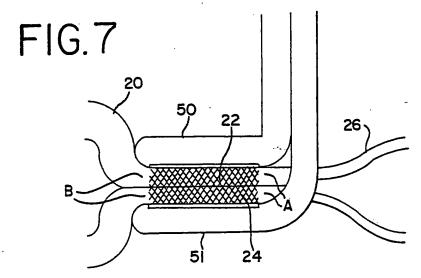



FIG.8

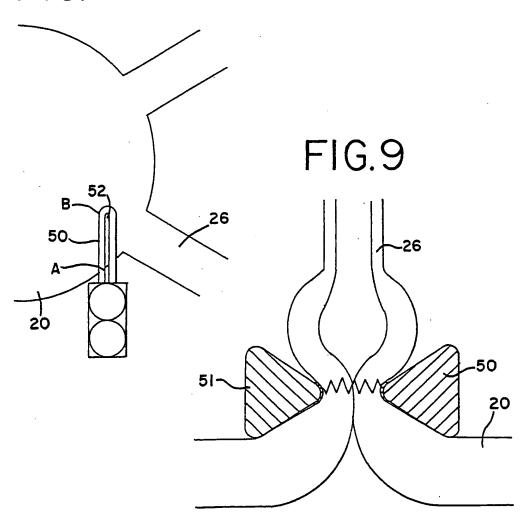



Michael D. Hooven et al.
Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 3 of 35


FIG.IO

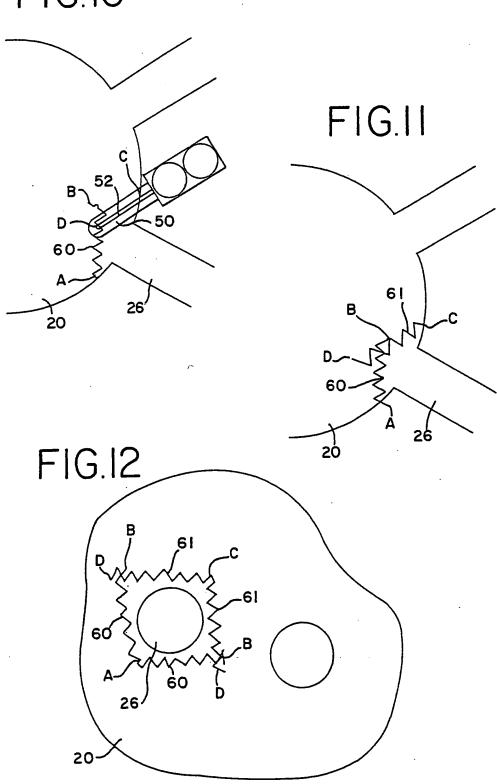

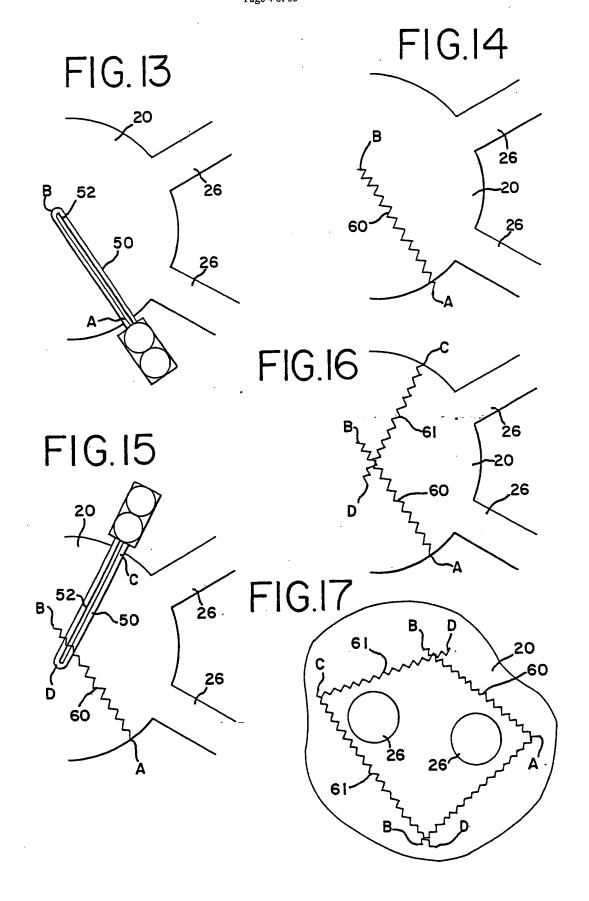

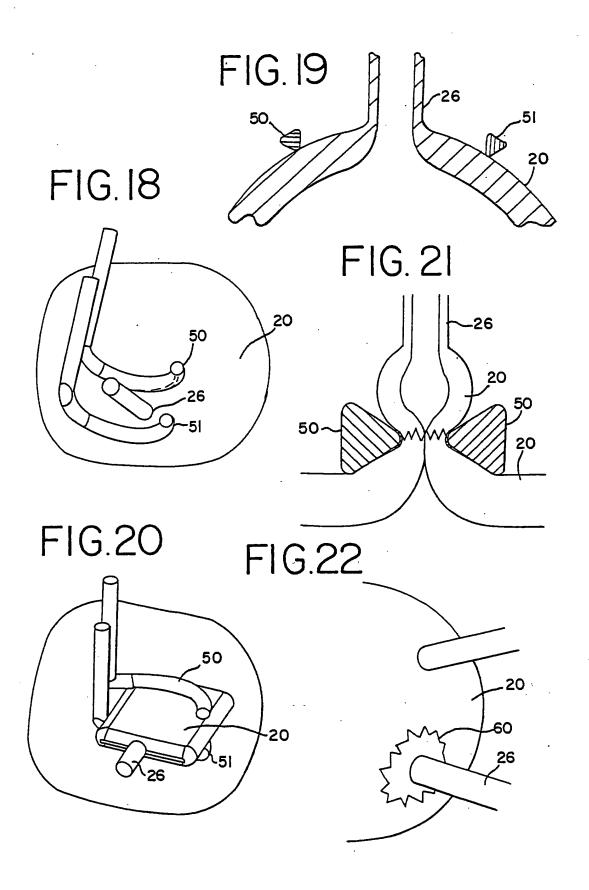


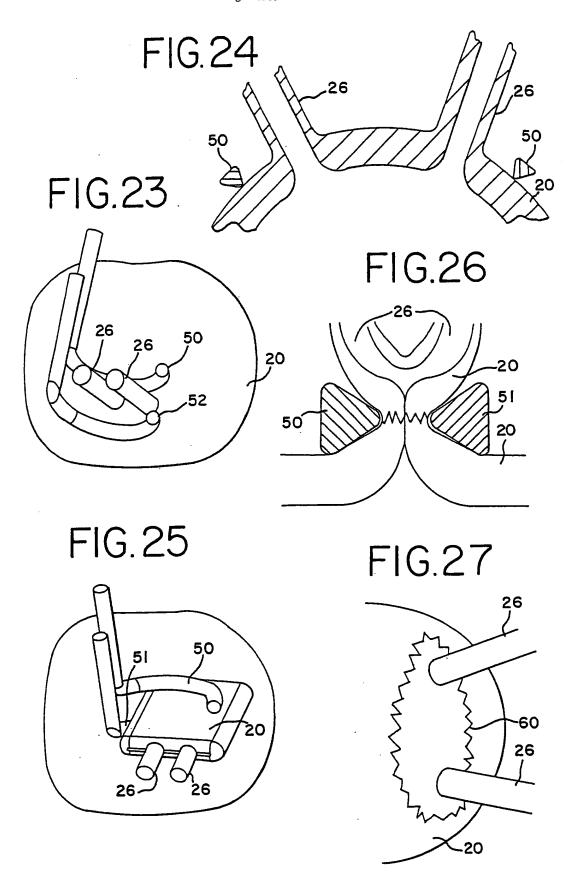


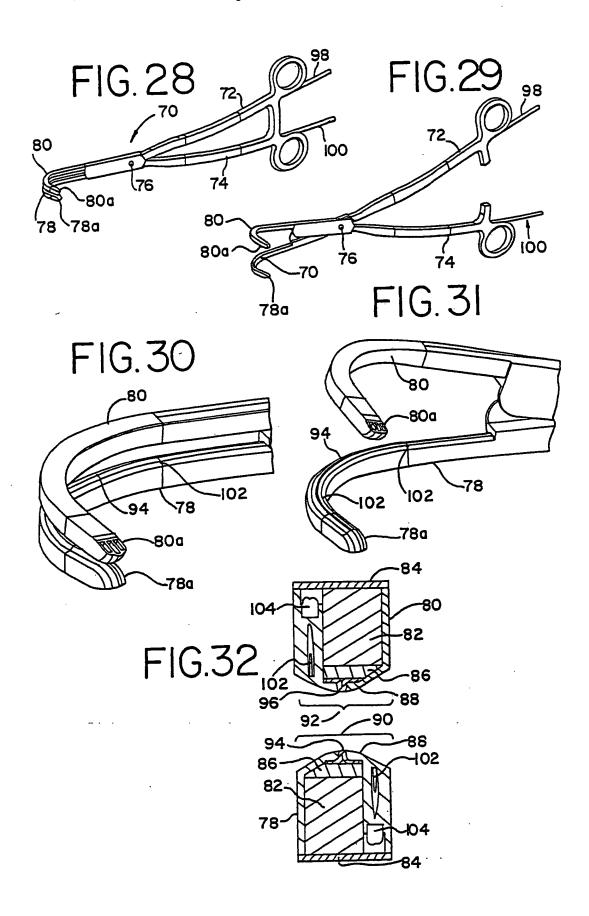

Michael D. Hooven et al.


Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 8 of 35

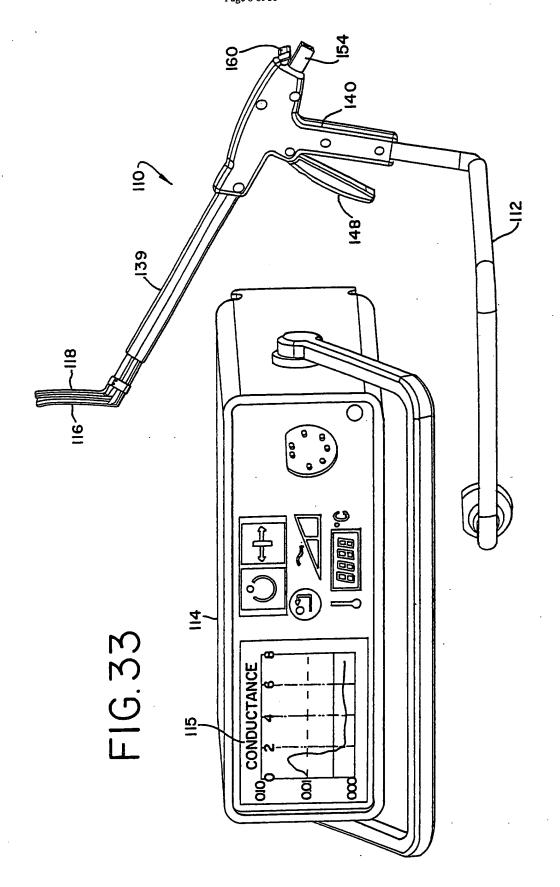

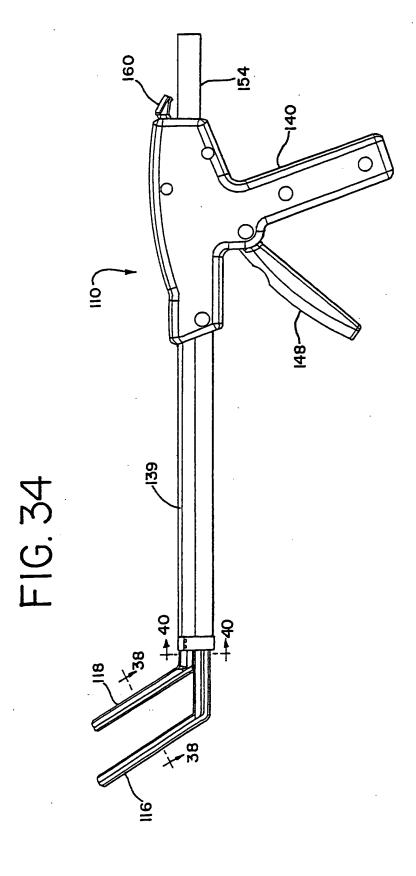

Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 10 of 35

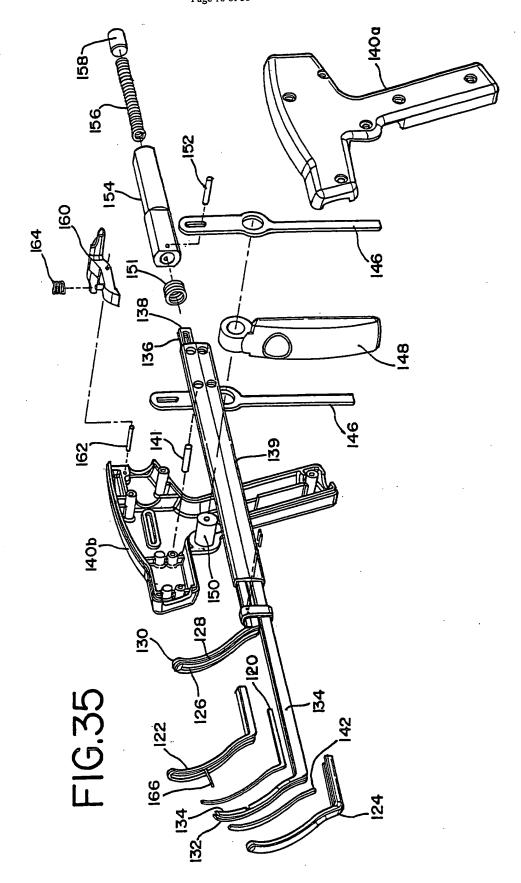

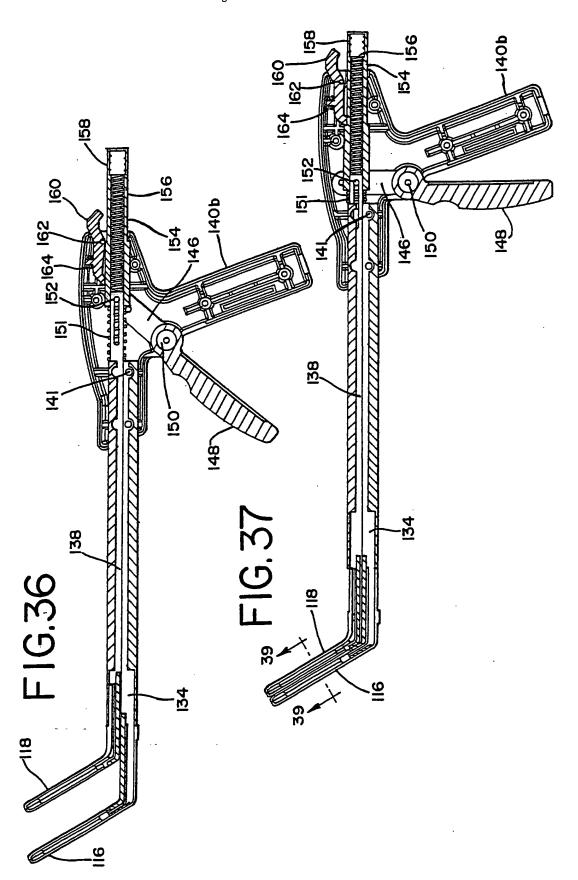


FIG.38

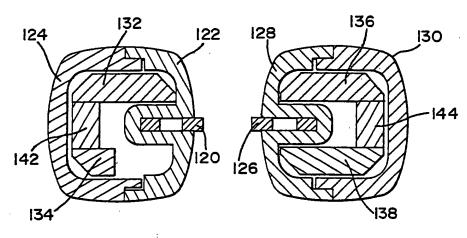


FIG. 39

124

142

144

144

FIG.40

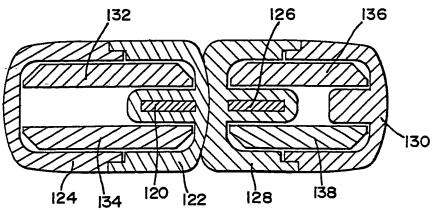


FIG.41




FIG.42




FIG.43




FIG.44




FIG.45







FIG.46



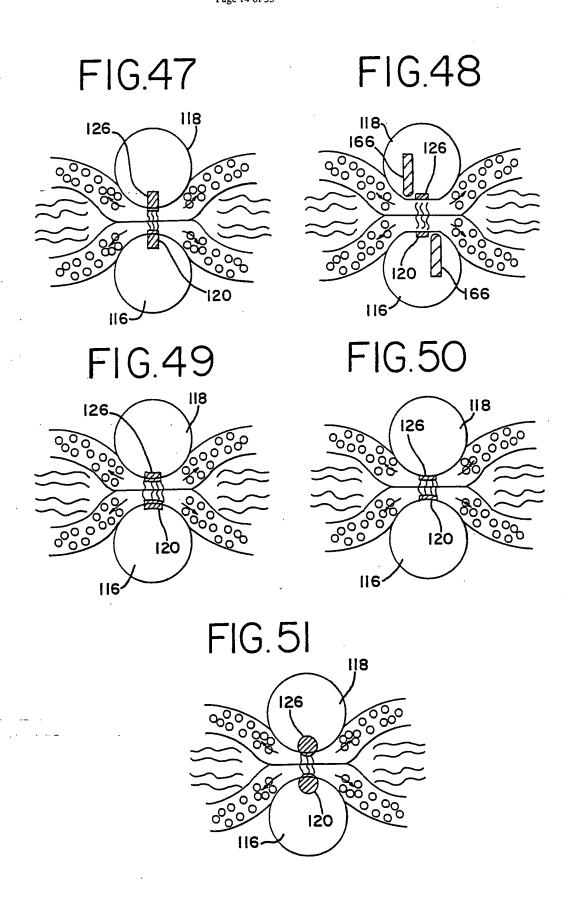

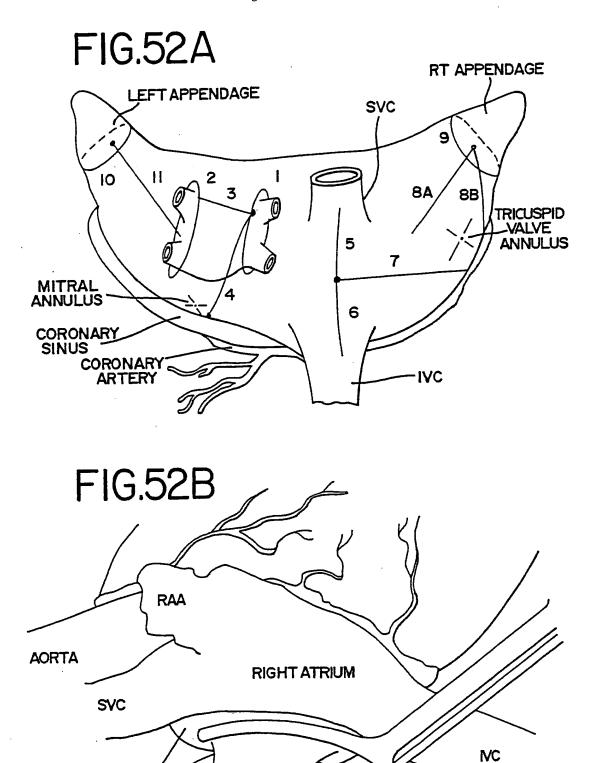



RPV'S

LEFT ATRIÚM

Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 16 of 35

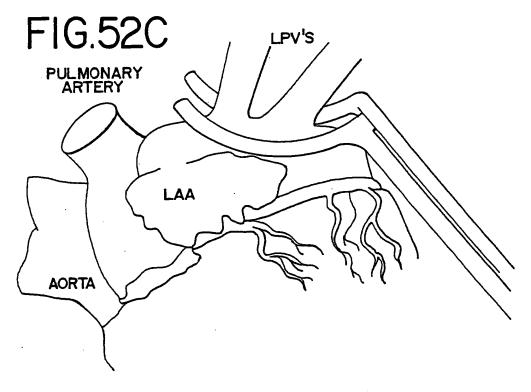

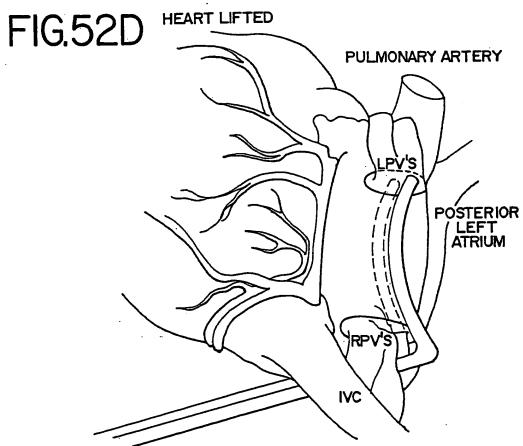




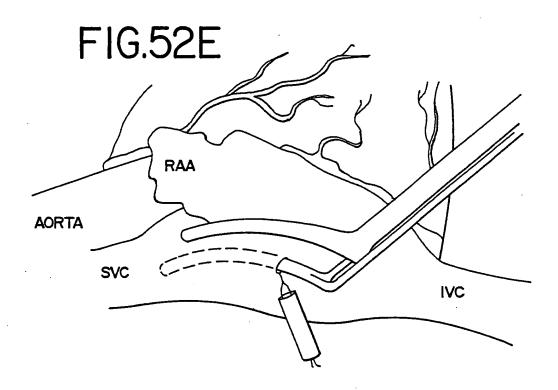


FIG.52F

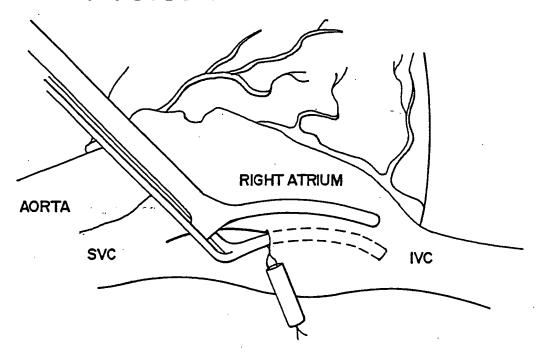


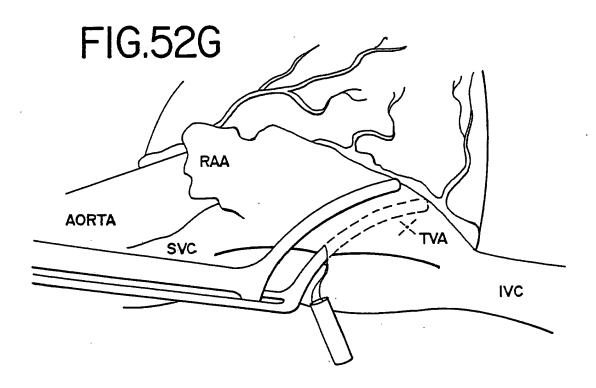


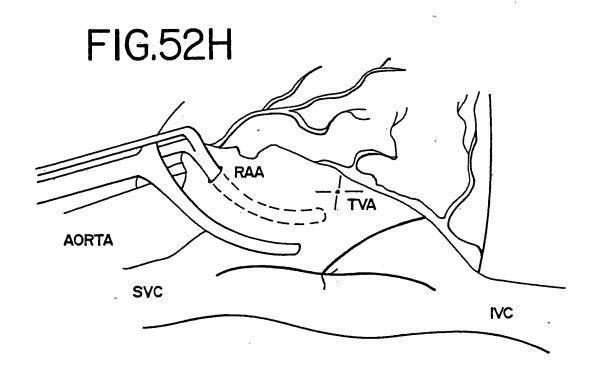

Michael D. Hooven et al.


Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 19 of 35

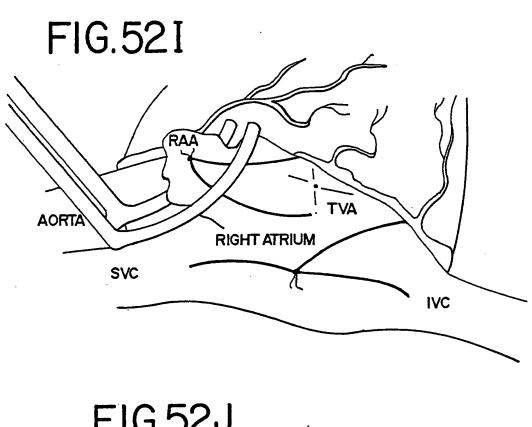

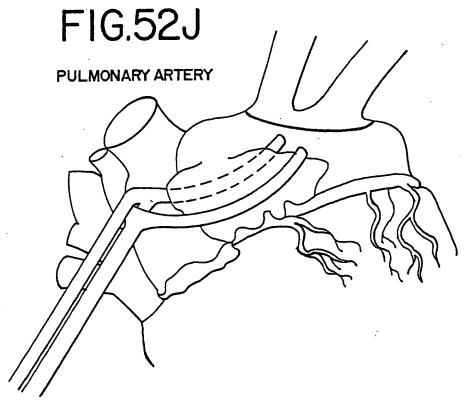



Michael D. Hooven et al.


Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 20 of 35

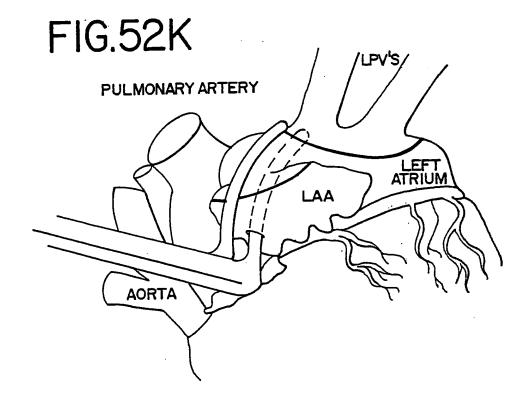

Michael D. Hooven et al.
Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 21 of 35

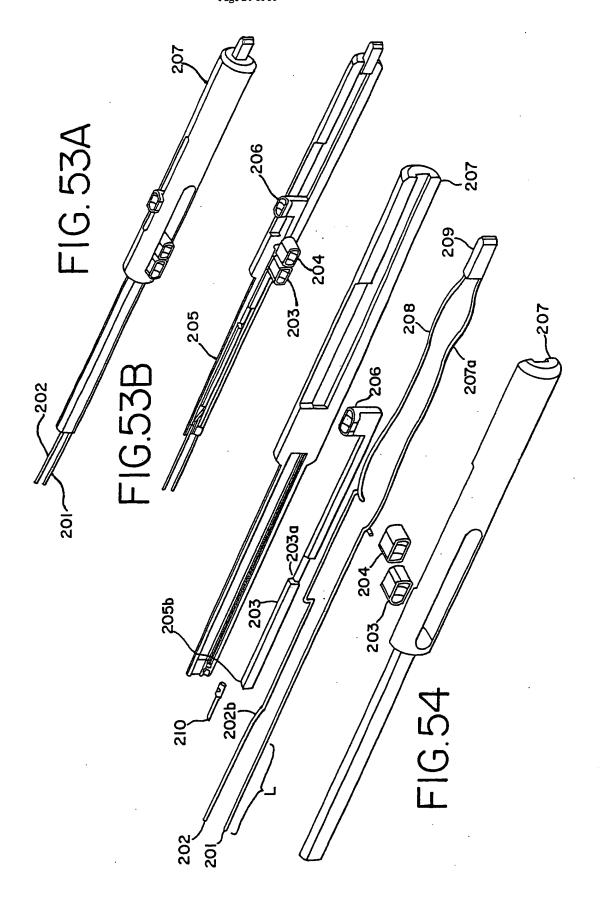

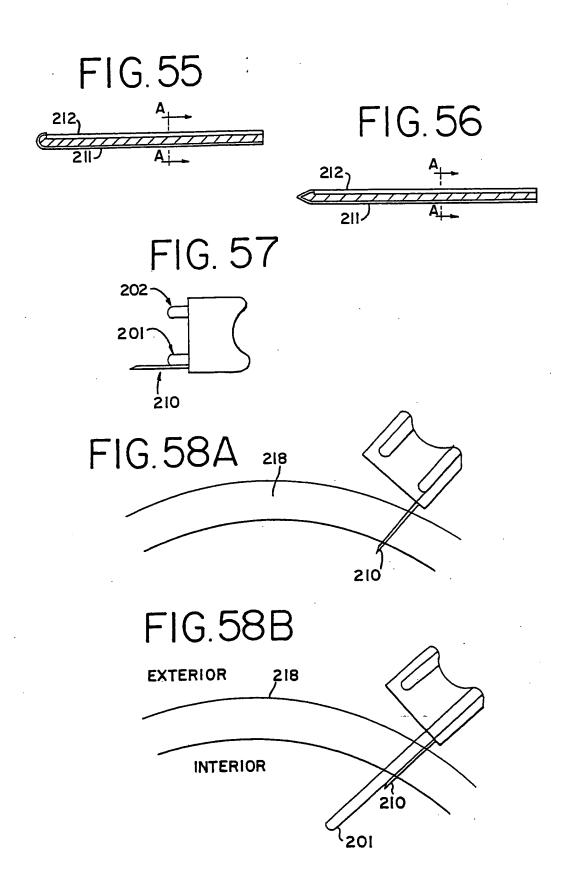

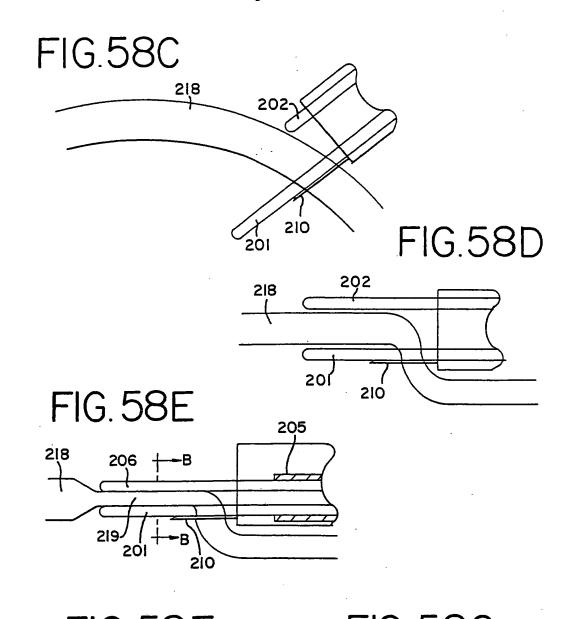




FIG. 58G




FIG. 59


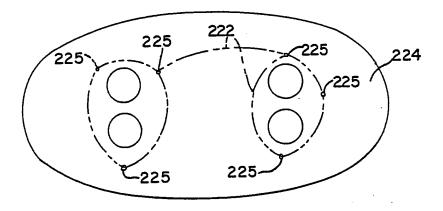


FIG. 60A

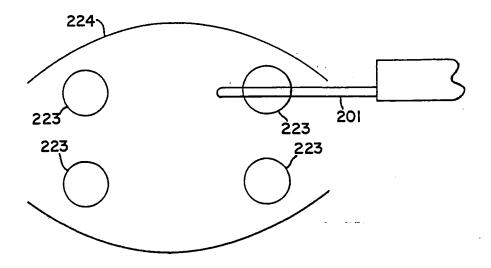

Michael D. Hooven et al. Transmural Ablation Device with Integral EKG Sensor Serial No. 10/032,378 0320-0012 Page 25 of 35

FIG. 60B




FIG.60C




FIG. 60D




FIG. 60E

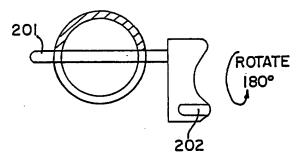


FIG.60F




FIG. 60G




FIG.60H






FIG. 601




Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 26 of 35

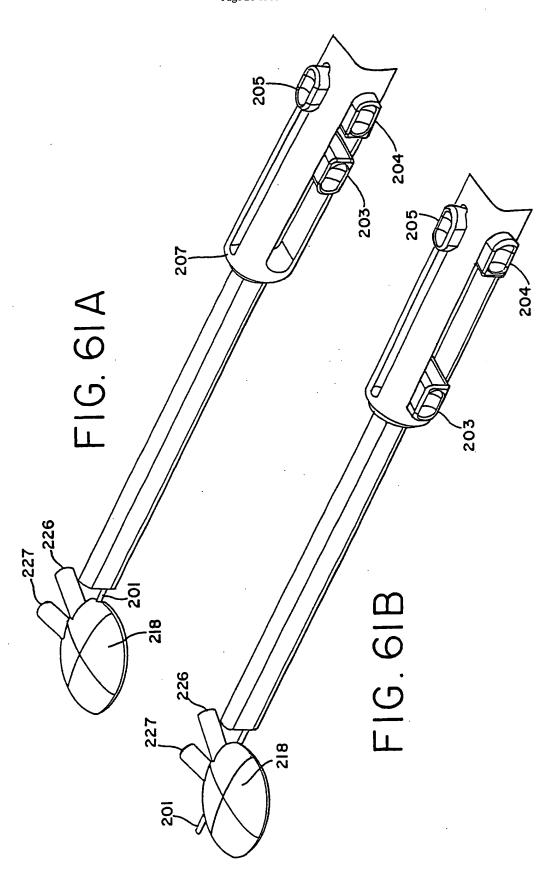


Michael D. Hooven et al.


Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 27 of 35

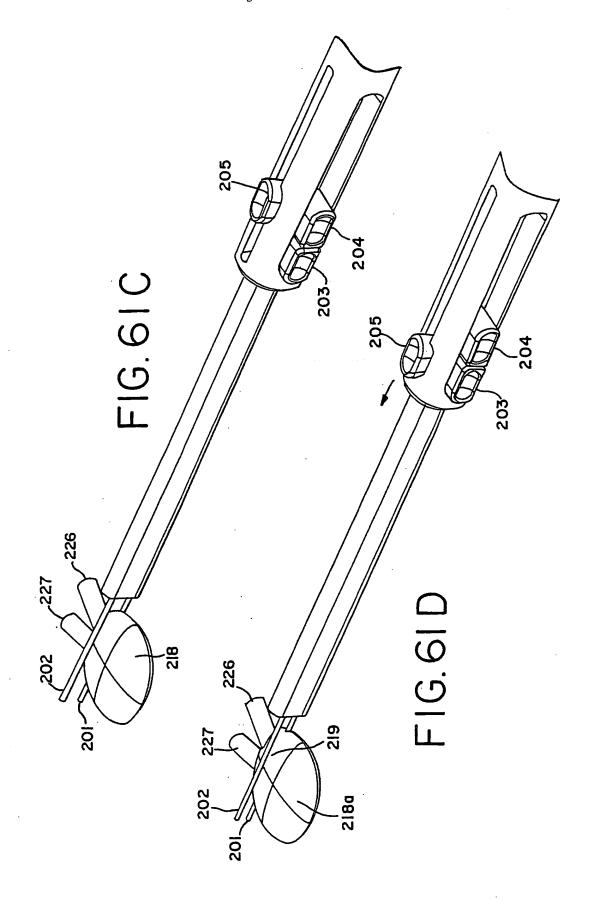


Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 28 of 35

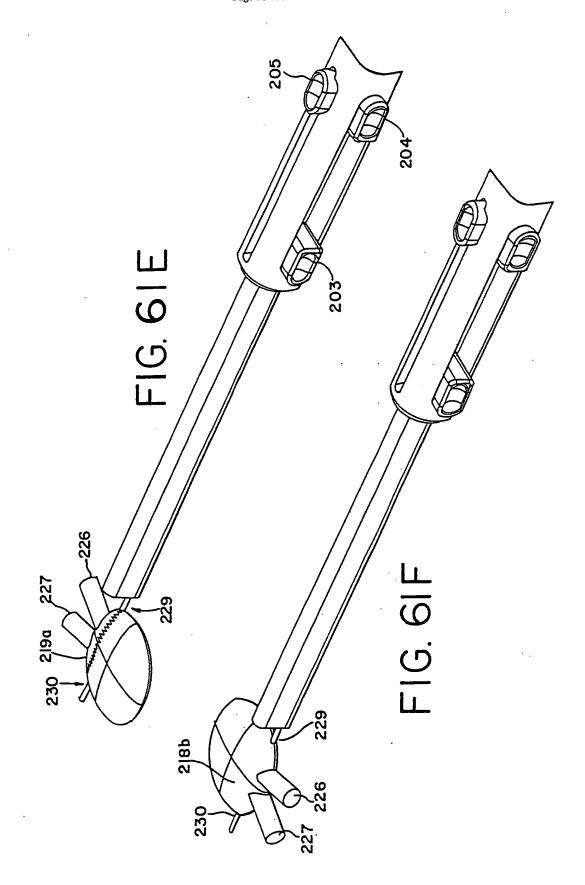

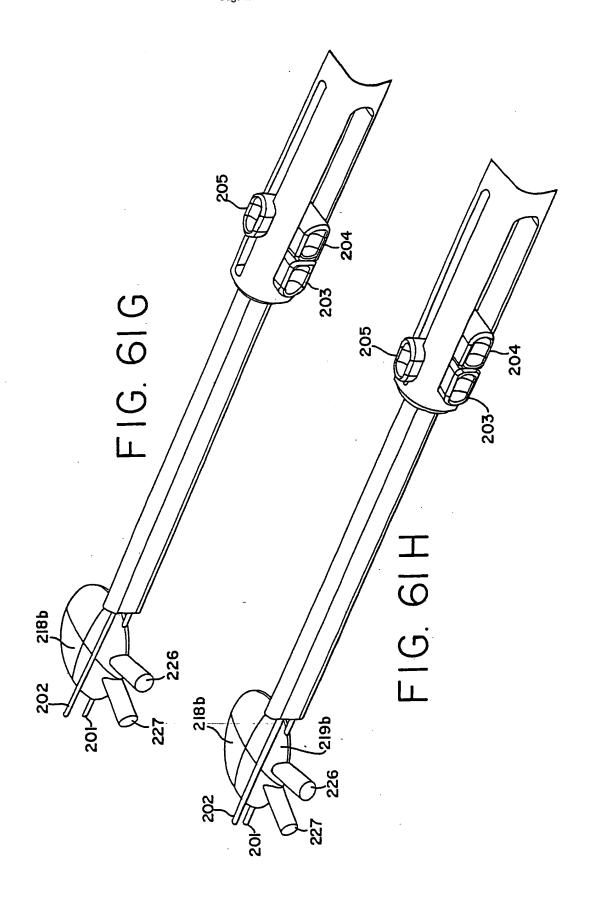

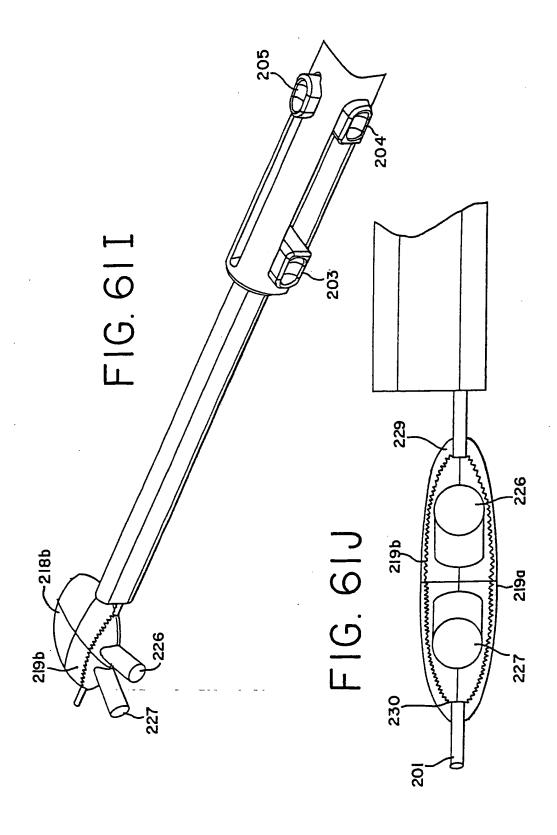

Michael D. Hooven et al.
Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 31 of 35

FIG.62A




FIG.62B





FIG.62C



Michael D. Hooven et al.
Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 32 of 35

FIG. 62D

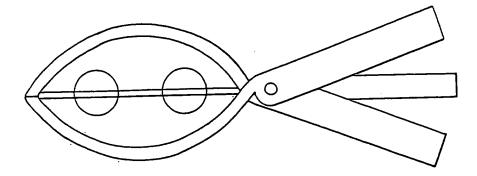


FIG. 62E



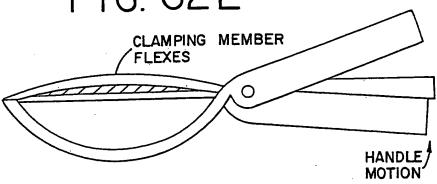



FIG. 62F



Michael D. Hooven et al.
Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 33 of 35

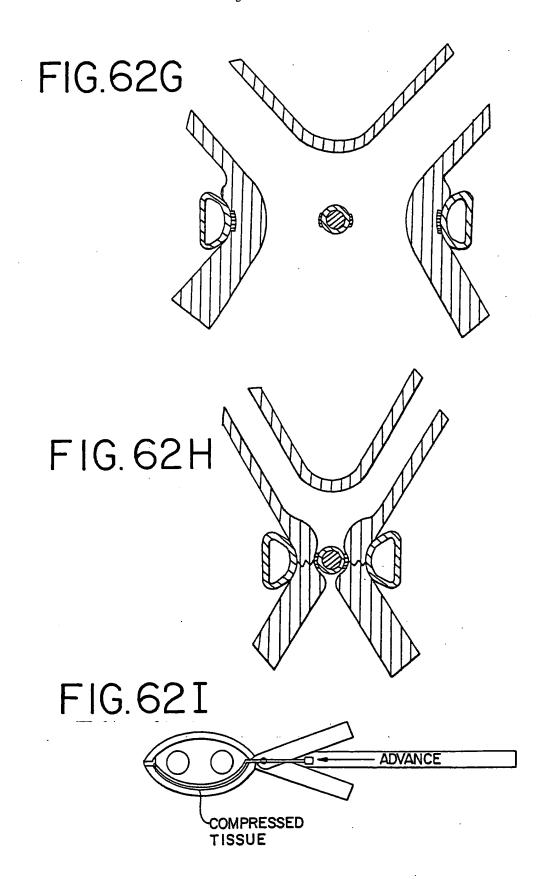

Michael D. Hooven et al. Transmural Ablation Device with Integral EKG Sensor Serial No. 10/032,378 0320-0012 Page 34 of 35

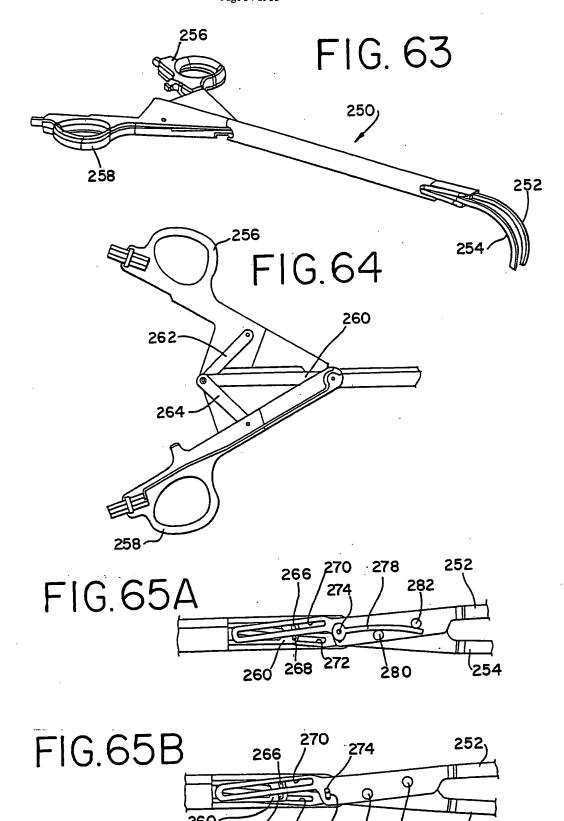

Michael D. Hooven et al.

Transmural Ablation Device with Integral EKG Sensor
Serial No. 10/032,378
0320-0012
Page 35 of 35

